 Attention | Do not let ink from pens, newspapers, product manual or other sources contact the manikin. Ink marks on the manikin will be irremovable.

**MW52** 

# **Female Catheterization/Enema Simulator II**

## **Instruction manual**

### **Contents**

---

- Introduction
  - Manufacturer's note/DOS and DON'TS . . . . . P.21
- Before you start
  - Set includes . . . . . P.22
- Preparation
  - Catheterization/Enema . . . . . P.23 ~ P.26
- Training session
  - Training session . . . . . P.27 ~ P.28
- After training . . . . . P.29 ~ P.33
- Replacement of consumable parts . . . . . P.34 ~ P.38
- FAQ s . . . . . P.39
- Precaution . . . . . P.40

## Manufacturer's note

This Female Catheterization/Enema Simulator has been developed for the training of medical and nursing professionals only. Any other use, or any use not in accordance with the enclosed instructions, is strongly discouraged. The manufacturer cannot be held responsible for any accident or damage resulting from such use. Please use this model carefully and refrain from subjecting to any unnecessary stress or wear. Should you have any questions on this simulator, please feel free to contact our distributor in your area or KYOTO KAGAKU at any time. (Our contact address is on the back cover of this manual)

### ● Features

- Basic high quality training in male and female: urethral catheterization, perineal care and enema.
- Form of genitalia, urethra, and bladder are anatomically correct.
- Successful insertion is confirmed by urine (water) outflow.
- Organ unit can be used separately, allowing training with SPs or full body manikins in clinical setting.

## ⚠ DOs and DON'Ts

### DOs

- Handle the manikin and the components with care.
- Storage in a dark, cool space will help prevent the skin colours from fading.
- The manikin skin may be cleaned with a wet cloth, if necessary, using mildly soapy water or diluted detergent.


### DON'Ts

- Do not let ink from pens, newspapers, product manual or other sources contact the manikin. Ink marks on the manikin will be irremovable.
- Never use organic solvent like paint thinner to clean the skin, as this will damage the simulator.
- Please use the genuine lubricant included in the set. Usage of other lubricants will cause damage to the model in a short time as in the following cases:
  - Jelly-type lubricants which remain in the model will harden and cause damage to the valves.
  - Water-soluble jelly-type lubricants will be washed out during urethral catheterization, which will decrease lubricating ability.

- The color of the tube or soft resin parts may change across the ages, but this does not affect the simulator use.


## Set Includes

Before your first use, ensure that you have all components listed below.

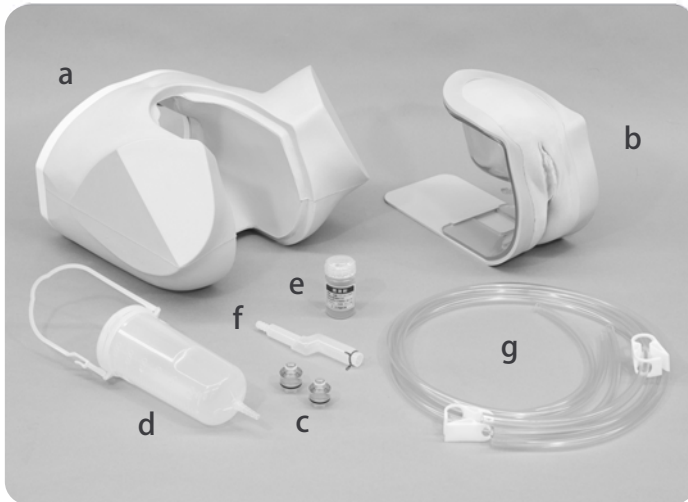

- a. Lower torso manikin ..... 1
  - b. Female genitalia organ unit ..... 1
  - c. Valve ..... 3  
(total 3 pcs; one is incorporated in the genitalia unit and two are for future replacement)
  - d. Irrigation bottle ..... 1
  - e. Lubricant ..... 1
  - f. Rectum unit ..... 1  
(attached with a metal clip 1)
  - g. Irrigation/drainage tubes ..... 3  
(total 3 pcs; 2 are attached with a clamp)
- Instruction manual

### Genitalia organ unit

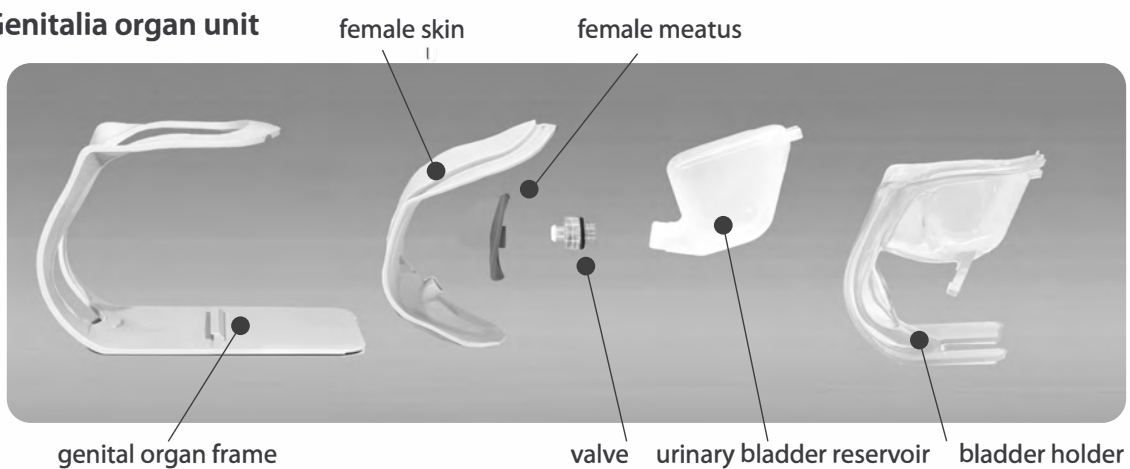

### Consumable parts

code	name
11381-300	replacement valve for MW2A/B (a set of 6)
11433-010	replacement female skin III
11433-020	replacement female meatus III(a set of 2)
11381-800	lubricant



11381-300



11433-020



11381-800



11433-010

### 1 Connection of Irrigation/drainage tubes


1. Remove the genitalia unit from the torso manikin.

Make room between torso manikin and the genitalia unit by opening the thighs. Then take out the genitalia unit from the torso manikin.





Genitalia unit

There are two tube connectors on the backside of the unit.

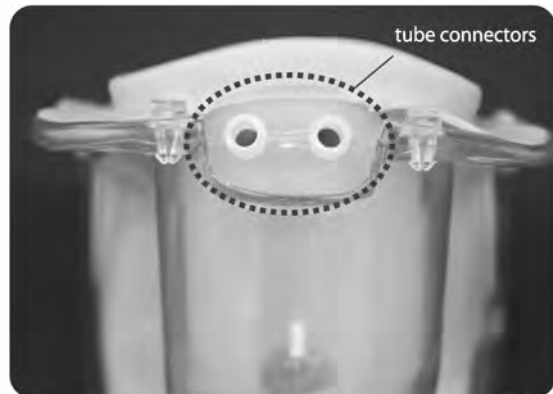

2. Attach the irrigation/drainage tubes with clamp to the connectors at the upper end of the urinary bladder reservoir.

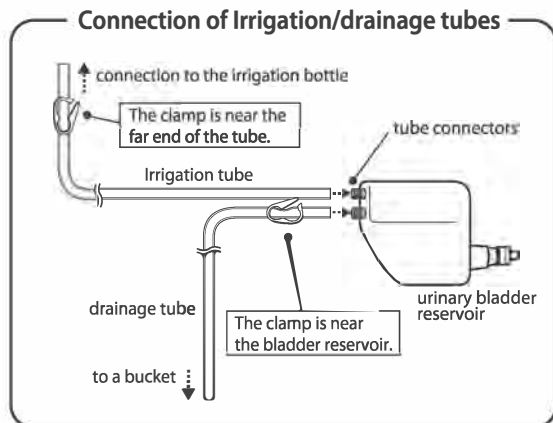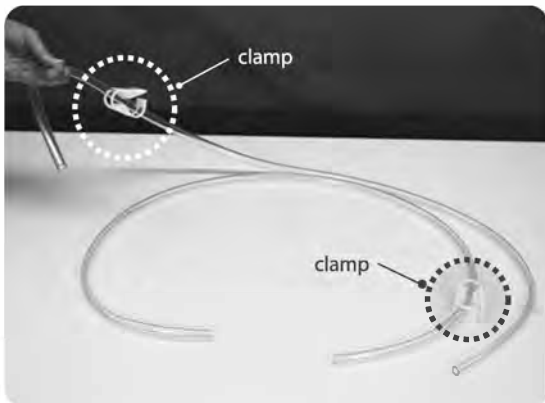


### 1 Connection of Irrigation/drainage tubes

3. One of the tube connectors is for irrigation and the clamp should be placed at the far end of the tube.



4. The other tube connector is for the drainage and the clamp on the tube should be placed around 20-30cm from the bladder.

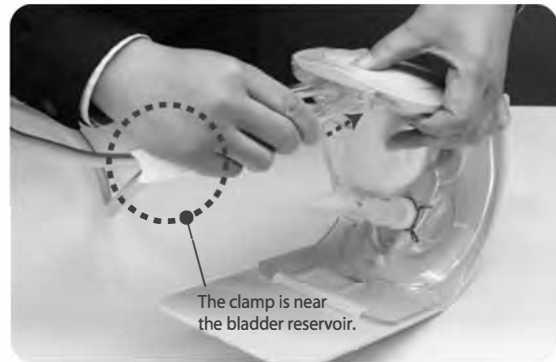

5. Connect the drain tube with no clamp to the rectum unit.



.....  
When attaching the tubes to the unit, hold the unit with one hand while inserting the tube to the port.



6. Set the genitalia units to the lower torso body.  
First put the 3 irrigation/drainage tubes through the body and then set the genitalia unit.



Assembly complete.

### 2 Connect the Irrigation bottle and fill the bladder with water

1. Connect the irrigation bottle to the irrigation tube which has clamp at near the far end.





2. Put the tip of drainage tubes for catheterization and enema into the bucket.





3. Close the clamp of irrigation tube before filling the bottle with water. And open the clamp of the drainage tube.

Irrigation tube

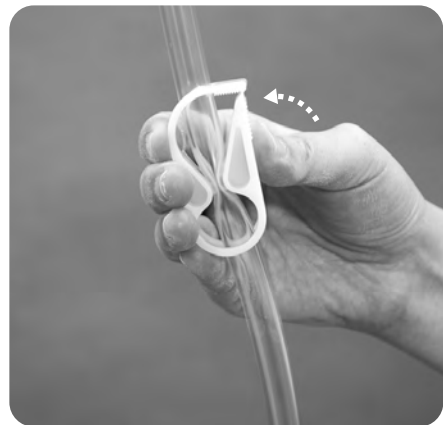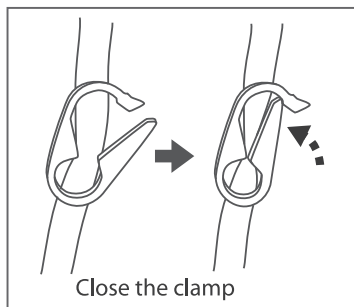


Drainage tube

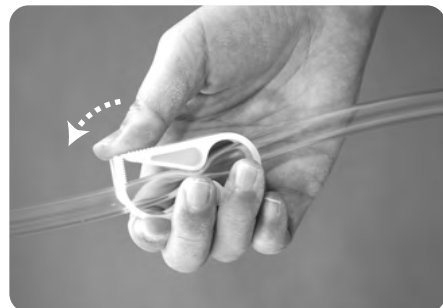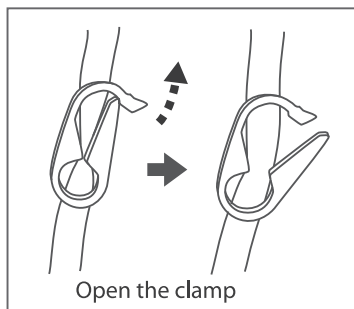

### 2 Connect the Irrigation bottle and fill the bladder with water


4. Fill the irrigation bottle with simulated urine (water). Then put the cap on the bottle and hang it from the stand.

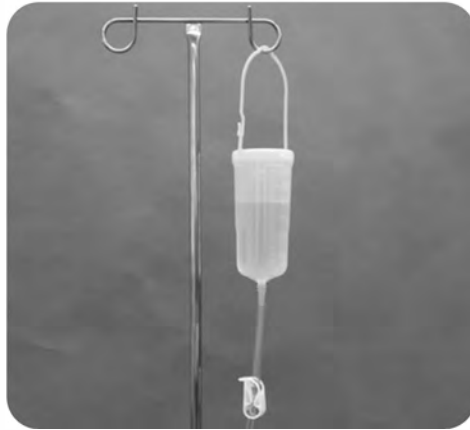

5. Open the clamp and the simulated urine will be charged into the bladder reservoir.



Irrigation tube

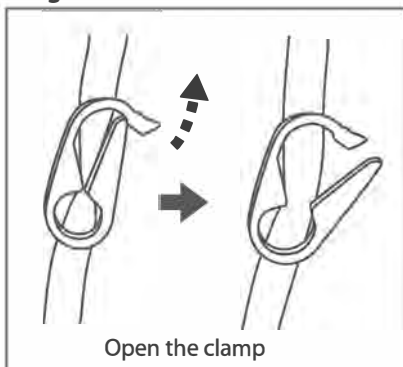

6. Ready.



## 1 Training procedure

### 1. Sterilizing of meatus urethra.

For training of sterilizing of meatus urethra, use water instead of actual antiseptic.

### 2. Inserting the catheter

Put the catheter in the tray, drip small quantity of lubricant to its tip. Ensure that about 5cm from the tip is coated by lubricant. Use the lubricant included in the set.



.....  
**Use 14-16Fr catheter for this model. Using larger catheter causes breakage of the valve.**  
**Please use the genuine lubricant included in the set. Usage of other lubricants will cause damage to the model in a short time as in the following cases:**

- Jelly-type lubricants which remain in the model will harden and cause damage to the valves.
- Water-soluble jelly-type lubricants will be washed out during urethral catheterization, which will decrease lubricating ability.

Product code of the genuine lubricant is 11381-800. Please refer to Page 22.

Simulated urine will be discharged when the catheter is inserted about 5cm. Before inflating the balloon, insert 2cm further from the point that first urine discharge is observed.



### 3. Removing the catheter

Discharge the water in the balloon before removing the catheter. Inflated balloon may cause breakage of the valve.



.....  
**The bladder reservoir needs to be refilled after EACH successful catheterization.**  
**In case water in the reservoir is low, water will not be flow out even when tip of the catheter reached in the bladder reservoir.**



## 2 Manual bladder compression


Close the clamps of the irrigation tube and drainage tube for manual bladder compression session.



The clamp of the irrigation tube



The clamp of the drainage tube

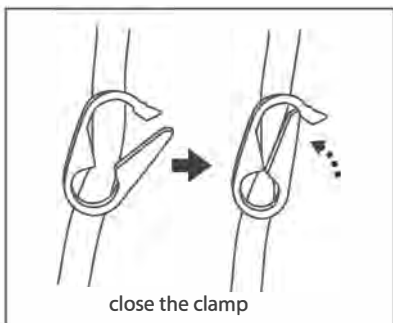

close the clamp



## 3 Training for enema

Do the training with left lateral position.



Use plenty amount of genuine lubricant for the training. Insufficient lubrication may cause the difficulty in the proper training.  
Enema tube cannot be inserted more than 7cm like real situation.



## 1 Drainage of water

1. Close the clamp of the irrigation tube. Drain the water from the irrigation bottle and tube.



2. Remove the genitalia unit from the torso body.

Make room between torso manikin and the genitalia unit by opening the thighs. Then take out the genitalia unit from the torso manikin.



3. Detach the rectum unit for enema training. Loosen the metal clip by tucking small wings together with fingers and remove the rectum unit from the hook of the bladder reservoir. Detach from the connector. Wash the rectum unit and let it dry naturally after the training sessions.



Caution

Always keep the clamp open for storage.





## 2 Drainage of water in the bladder reservoir

1. Disassemble the genitalia unit.

a) The genital organ frame and the bladder holder are fixed with two notches and nail shaped fasteners. To disengage the parts, lift the genital organ frame with fingers.



b) Remove the skin with the bladder holder from the outer frame. Then peel the skin from the bladder holder.

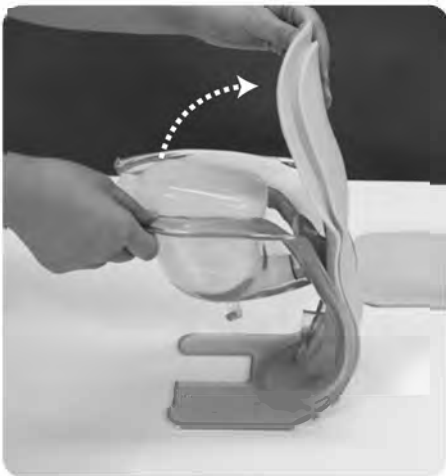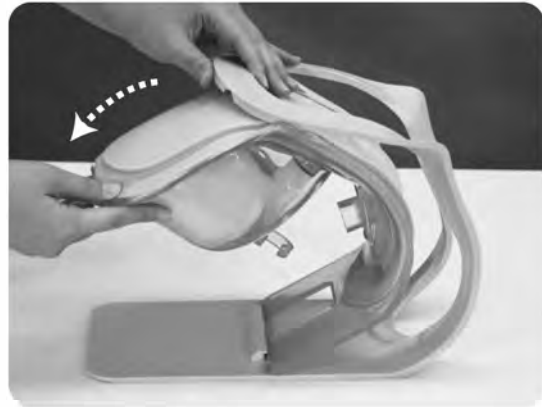

2. Remove the bladder reservoir from the bladder holder. Detach the irrigation and drainage tubes. Then detach the female meatus from the valve. Then drain the water from the reservoir.



Do this procedure over the sink.

## 3 Assembly for storage




1. After the training, wipe the valve and the meatus urethra thoroughly.  
Wipe the joint between the valve and the meatus urethra to remove the lubricant, using mildly soapy water and let it dry naturally.

2. Attach the meatus urethra.




3. Set the bladder in the bladder holder.

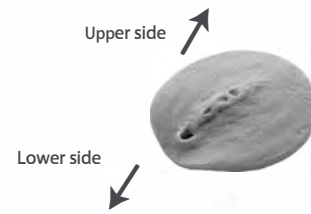


⚠ Caution

Take care to set the meatus urethra in correct direction.

4. Insert the projection of the bottom of the skin in the lower hole of the bladder holder.

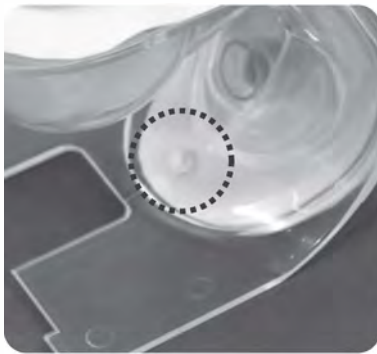


5. Put the skin over the bladder holder and insert two upper projections of the skin in two upper holes of the bladder holder.

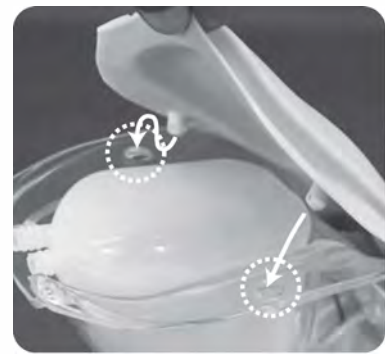

## 3 Assembly for storage

7. Set the bladder holder to the genital organ frame.

a) Set the lower edge of bladder holder to the stopper on the frame. Then, holding the frame firmly, push the holder forward.

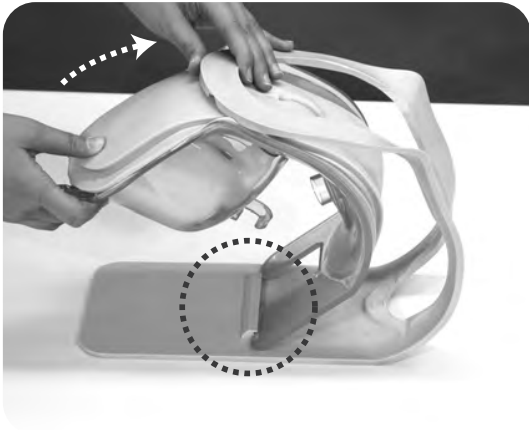

b) To fit the upper side of the skin in the genital organ frame, tuck the skin under the frame with fingers.



c) Then engage the frame and holder by pushing the corner of the genital organ frame forward (to the abdomen side), until clicking sound is heard.



Or, support the fasteners from the back side by fingers and draw the genital organ frame over it toward you.




## 3 Assembly for storage

8. Connect the rectum unit.

Set the rectum unit to the tube connector of the genitalia unit.



.....  
Set the rectum unit with correct angle as shown in the picture.

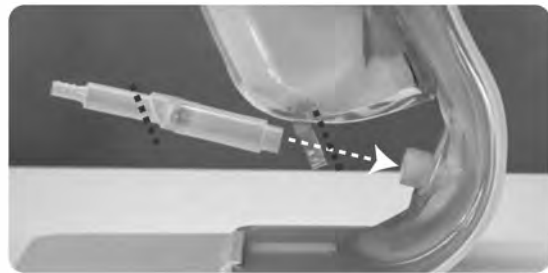

9. Secure the rectum unit with the metal clip.



10. Set the genitalia unit to the lower torso model.



## 1 Disassemble the unit

1. Remove the genitalia unit from the torso body.

Make room between torso manikin and the genitalia unit by opening the thighs. Then take out the genitalia unit from the torso manikin.



2. Detach the rectum unit for enema training. Loosen the metal clip by tucking small wings together with fingers and remove the rectum unit from the hook of the bladder reservoir. Detach from the connector.



**Caution**

Support and hold tube connector port when removing the rectum unit.

3. Disassemble the genitalia unit.

a) The genital organ frame and the bladder holder are fixed with two notches and nail shaped fasteners. To disengage the parts, lift the genital organ frame with fingers.




b) Remove the skin with the bladder holder from the outer frame. Then peel the skin from the bladder holder.



## 1 Disassemble the unit

c) Peel the skin from the bladder holder.

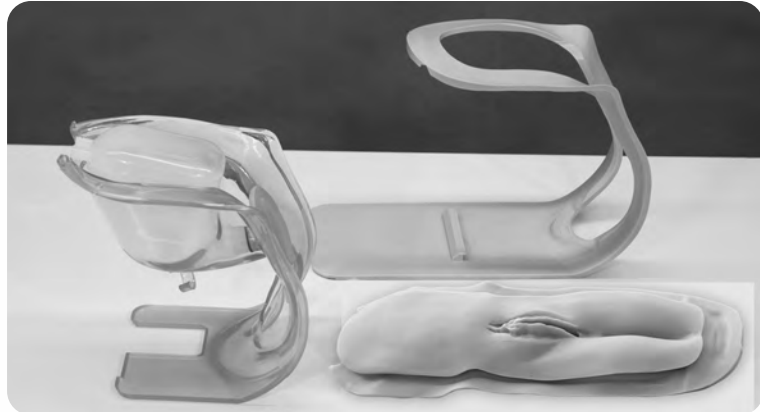

4. Remove the bladder reservoir from the bladder holder. Detach the meatus urethra from the valve.



 Caution

.....  
Replace the genitalia skin and the meatus urethra at this moment.


5. Unscrew the valve from the bladder reservoir.



## 2 Replacement of the valve



1. Replace the valve and screw it to the bladder reservoir.


 Caution

.....  
Ensure that rubber seal is set on the valve, before screw it to the bladder reservoir.



## 3 Replacement of the skin and meatus urethra

1. Set the new meatus urethra part to the valve.




2. Set the bladder in the bladder holder.




 Caution

.....  
Take care to set the meatus urethra in correct direction.

3. Insert the projection at the bottom of the skin in the lower hole of the bladder holder.

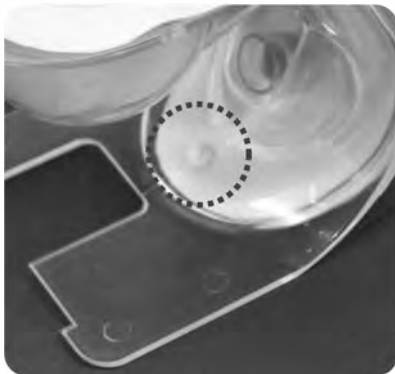


4. Put the skin over the bladder holder and insert two upper projections of the skin in two upper holes of the bladder holder.

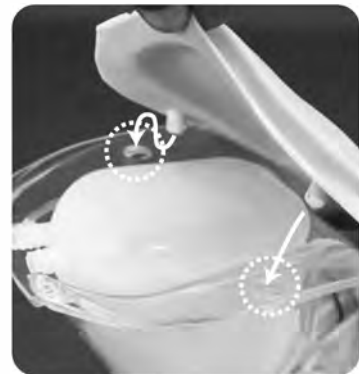

## 4 Assembly for storage

1. Set the bladder holder to the genital organ frame.

a) Set the lower edge of bladder holder to the stopper on the frame. Then, holding the frame firmly, push the holder forward.

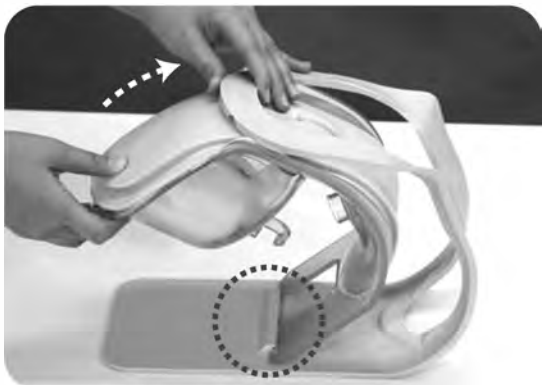

b) To fit the upper side of the skin in the genital organ frame, tuck the skin under the frame with fingers.



c) Then engage the frame and holder by pushing the corner of the genital organ frame forward (to the abdomen side), until clicking sound is heard.



Or, support the fasteners from the back side by fingers and draw the genital organ frame over it toward you.



## 4 Assembly for storage

2. Connect the rectum unit.

Set the rectum unit to the tube connector of the genitalia unit. Then set it on the hook.



.....  
Set the rectum unit with correct angle as shown in the picture.



3. Secure the rectum unit with the metal clip.



4. Set the genitalia unit to the lower torso model.



## FAQ s

Quick check-up before calling the customer service, when the you have problems in using the simulator. Look in the "cases" section for a description of the problem to find a possible solution.

### Catheterization training

Cases	Reason	Solution
Water leakage	The valve is worn.	Replace it with the new valve
	Loose connection of the valve and bladder reservoir or meatus urethra.	Check the connection of the valve and bladder or meatus urethra, reconnect them tightly.
Water does not come out when the catheter is inserted.	Water in the bladder reservoir is low.	Fill water into the bladder reservoir by using irrigation bottle.
	Clamps of the irrigation and drainage tubes are closed.	Open the both clamps of irrigation and drainage tubes.
Valve is easily damaged	Using a non-genuine lubricant that is not included in the set.	Use the lubricant included in the set.
	Using a catheter larger than the recommended size.	Use a catheter of the recommended size of 14-16 Fr.

### Enema Training

Cases	Reason	Solution
Glycerin enema tube can be inserted more than 7cm.	Connection of the genitalia organ unit and rectum unit is not correct.	Confirm the connection of the genitalia organ unit and rectum unit. Then set them steadily.
Water leakage		Ensure that the metal clips securing the genitalia organ and rectum unit are firmly in place.

# Precaution

## Some parts of MW2B are not common with MW52

Following parts of MW2B are not compatible with MW52 due to differences in their size or structures.


Metal clip for the rectum unit: the clip for MW52 is smaller



For MW2B  
(skin 11381-610)

For MW52  
(11433-010)

Female skin: Skin for MW52 is softer and with labia

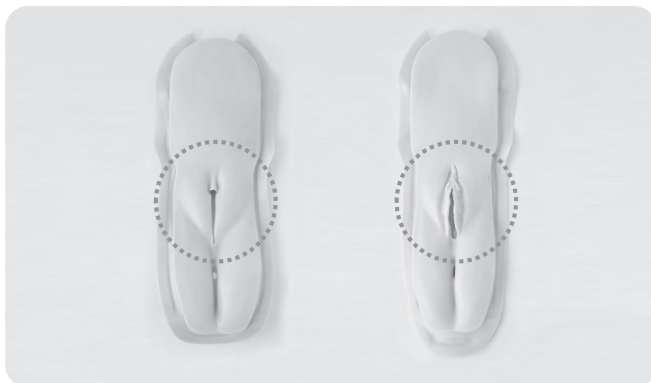

For MW2B  
(11381-610)

For MW52  
(11433-010)

Female meatus: Meatus for MW52 is without labia



For MW2B  
(11381-700)



For MW52  
(11433-020)



**注意**

モデル表面に印刷物などが直接触れないようにしてください。  
樹脂にインクが吸収されて消えなくなります。



**Caution**

Do not let ink from pens, newspapers, product manual or other sources contact the manikin. Ink marks on the manikin will be irremovable.

- 本製品についてのお問い合わせや不具合等ございましたら、お手数ですがお買い上げの販売店、もしくは下記（株）京都科学まで御連絡ください。
- For inquiries and service, please contact your distributor or KYOTO KAGAKU CO., LTD.



URL・<http://www.kyotokagaku.com> e-mail・[rw-kyoto@kyotokagaku.co.jp](mailto:rw-kyoto@kyotokagaku.co.jp)

■ 本社・工場

〒612-8388 京都市伏見区北寝小屋町15番地  
TEL: 075-605-2510 (直通)  
FAX: 075-605-2519

■ 東京支店

〒113-0033 東京都文京区本郷三丁目26番6号  
NREG本郷三丁目ビル2階  
TEL: 03-3817-8071 (直通)  
FAX: 03-3817-8075

■ Main Office and Factory (World Wide)

 **KYOTO KAGAKU co.,LTD**

WEB・[www.kyotogagaku.com](http://www.kyotogagaku.com)

E-MAIL・[rw-kyoto@kyotokagaku.co.jp](mailto:rw-kyoto@kyotokagaku.co.jp)

15 kitane-koya-cho Fushimi-ku Kyoto 612-8388, Japan  
TEL: +81-75-605-2510  
FAX: +81-75-605-2519

■ North and South American regions:



**KK America**  
Kyoto Kagaku America Inc.

WEB・[www.kkamerica-inc.com](http://www.kkamerica-inc.com)

E-MAIL・[info@kkamerica-inc.com](mailto:info@kkamerica-inc.com)

3109 Lomita Boulevard, Torrance, CA 90505-5108, USA  
TEL: +1-310-325-8860  
(Toll-free in North America: 877-648-8195)  
FAX: +1-310-325-8867

本書の内容は、予告なしに変更することがあります。本書の内容の一部もしくは全部を当社に無断で複写・転載することを禁じます。

本書の内容に、万一不審な点や誤りなど、お気づきの点がございましたら、当社もしくは販売店にご連絡ください。

The contents of the instruction manual are subject to change without prior notice.

No part of this instruction manual may be reproduced or transmitted in any form without permission from the manufacturer.

Please contact manufacturer for extra copies of this manual which may contain important updates and revisions.

Please contact manufacturer with any discrepancies in this manual or product feedback. Your cooperation is greatly appreciated.